
ANALYT MESSTECHNIK

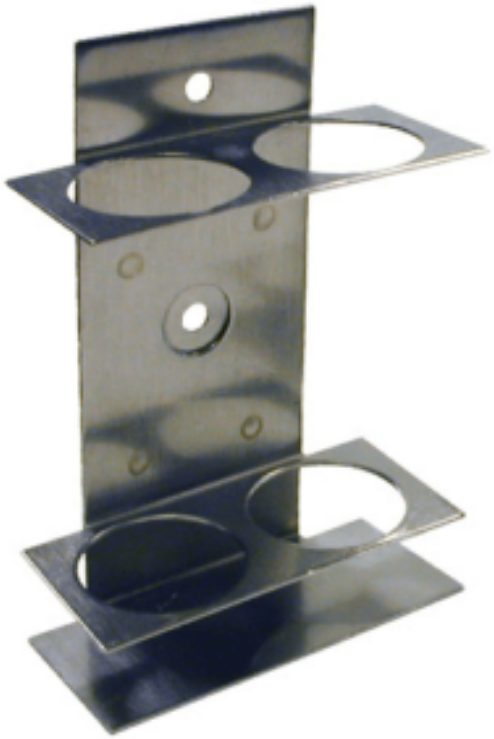

INSTRUCTIONS FOR USE

SKC Impinger Holders 225-20 for AirChek TOUCH Series Pumps

How to attach the SKC midget impinger holders 225-20-03, 225-20-04, 225-20-05 and 225-20-06 to the belt clip of an SKC AirChek TOUCH series sample pump.

AMTC-IN-0034

About this document

An SKC midget impinger holder of the 225-20 series carries your impingers on the sample pump itself. These instructions show how to attach the holder to the belt clip of an SKC AirChek TOUCH series sample pump.

Product and supplied items (p. 4) lists the holders this applies to and Before use (p. 5) takes you through the two steps. Filling the impingers, connecting the tubing and setting the flow rate are not covered; follow the instructions for your impingers, your pump and the method you sample to.

Keep these instructions for the lifetime of the product. The current revision is on the product page at analyt-mtc.com.

Document information

Title	SKC Impinger Holders 225-20 for AirChek TOUCH Series Pumps — Instructions for use
Document number	AMTC-IN-0034
Revision	Rev. 2 — October 2026
Applies to	SKC midget impinger holders 225-20-03, 225-20-04, 225-20-05 and 225-20-06
Language	English
Manufacturer	SKC Inc.

Revision history

Rev.	Date	Change
2	October 2026	Quality programme: new document type, number and identity pages.
1	October 2026	First issue.

SKC and AirChek are trademarks of their owners. Information in these instructions is subject to change without notice. © 2026 ANALYT-MTC Messtechnik GmbH. All rights reserved.

Contents

1 **Product and supplied items** 4
Holders covered 4

2 **Before use** 5
Attaching the holder 5

3 **Ordering information** 6

4 **Service and contacts** 7
Disposal 7

CHAPTER 1

Product and supplied items

Holders covered

Holder	Order code
Double holder for glass midget impingers	225-20-03
Single holder for glass midget impingers	225-20-05
Holder for PFA midget impingers	225-20-04, 225-20-06

The figures show the 225-20-03, a stainless steel double holder that takes two glass impingers, or one impinger and one trap. SKC gives one fitting procedure for the whole series: the holder has a toggle on its back that locks into the slot of the pump belt clip.

To use a trap in the holder, fill it and replace its sorbent as the guide *SKC Impinger Traps 225-22 and 225-22-01 — Instructions for use* (AMTC-IN-0044) describes.

CHAPTER 2

Before use

Attaching the holder

1. Hold the holder on its side. Push the toggle on its back into the slot in the pump belt clip.

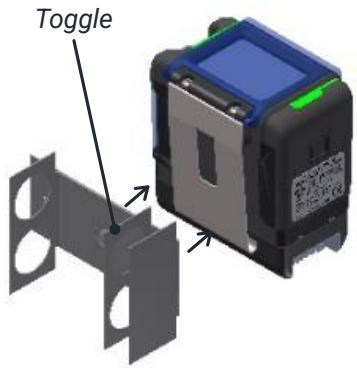


Figure 2-1. Toggle into the slot.

2. Turn the holder through 90 degrees. The toggle now catches on both sides of the slot and holds the holder firmly on the pump.
3. Check the position: the bottom plate of the holder lies parallel with the bottom of the pump.



Figure 2-2. Holder fitted, bottom plate parallel with the pump.

CHAPTER 3

Ordering information

Order from Analyt-MTC with the order codes.

The holders and their order codes are listed in Product and supplied items (p. 4). For holders, impingers and traps, ask Analyt-MTC.

CHAPTER 4

Service and contacts

Contact and support

ANALYT-MTC Messtechnik GmbH

German Headquarters

Klosterrunsstraße 18, 79379 Müllheim
Germany

+49 7631 5545

info@analyt-mtc.de

French Subsidiary

175 Avenue d'Alsace, 68000 Colmar
France

+33 3 89 41 47 78

info@analyt-mtc.fr

www.analyt-mtc.com

Before you call

Have the following at hand so Analyt-MTC can help you quickly:

- the catalogue number of the holder, for example 225-20-03;
- the model of the sample pump the holder is fitted to;
- the impingers or trap you use in the holder, glass or PFA.

Analyt-MTC handles technical questions, warranty matters and returns under its terms of sale; its contact details are above and on the back cover.

Disposal

Dispose of the holder under local regulations; separate metal, glass and plastic parts for recycling where possible.

ANALYT-MTC Messtechnik GmbH

Sales, service and calibration

German Headquarters
Klosterrunsstraße 18, 79379 Müllheim
Germany
+49 7631 5545
info@analyt-mtc.de

French Subsidiary
175 Avenue d'Alsace, 68000 Colmar
France
+33 3 89 41 47 78
info@analyt-mtc.fr

www.analyt-mtc.com

AMTC-IN-0034 · Rev. 2 · 2026-10

© 2026 ANALYT-MTC Messtechnik GmbH. All rights reserved. Subject to technical changes without notice.